Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation/Operation Instructions

9A430XX CHAIR ARM SET ASSEMBLY

KIT COMPONENTS

Part Number	Description	Qty.
9A430XX	Chair Arm Set	1 pair
003-0932-00	Installation / Operation Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To provide support and comfort to patient during general examinations.

1

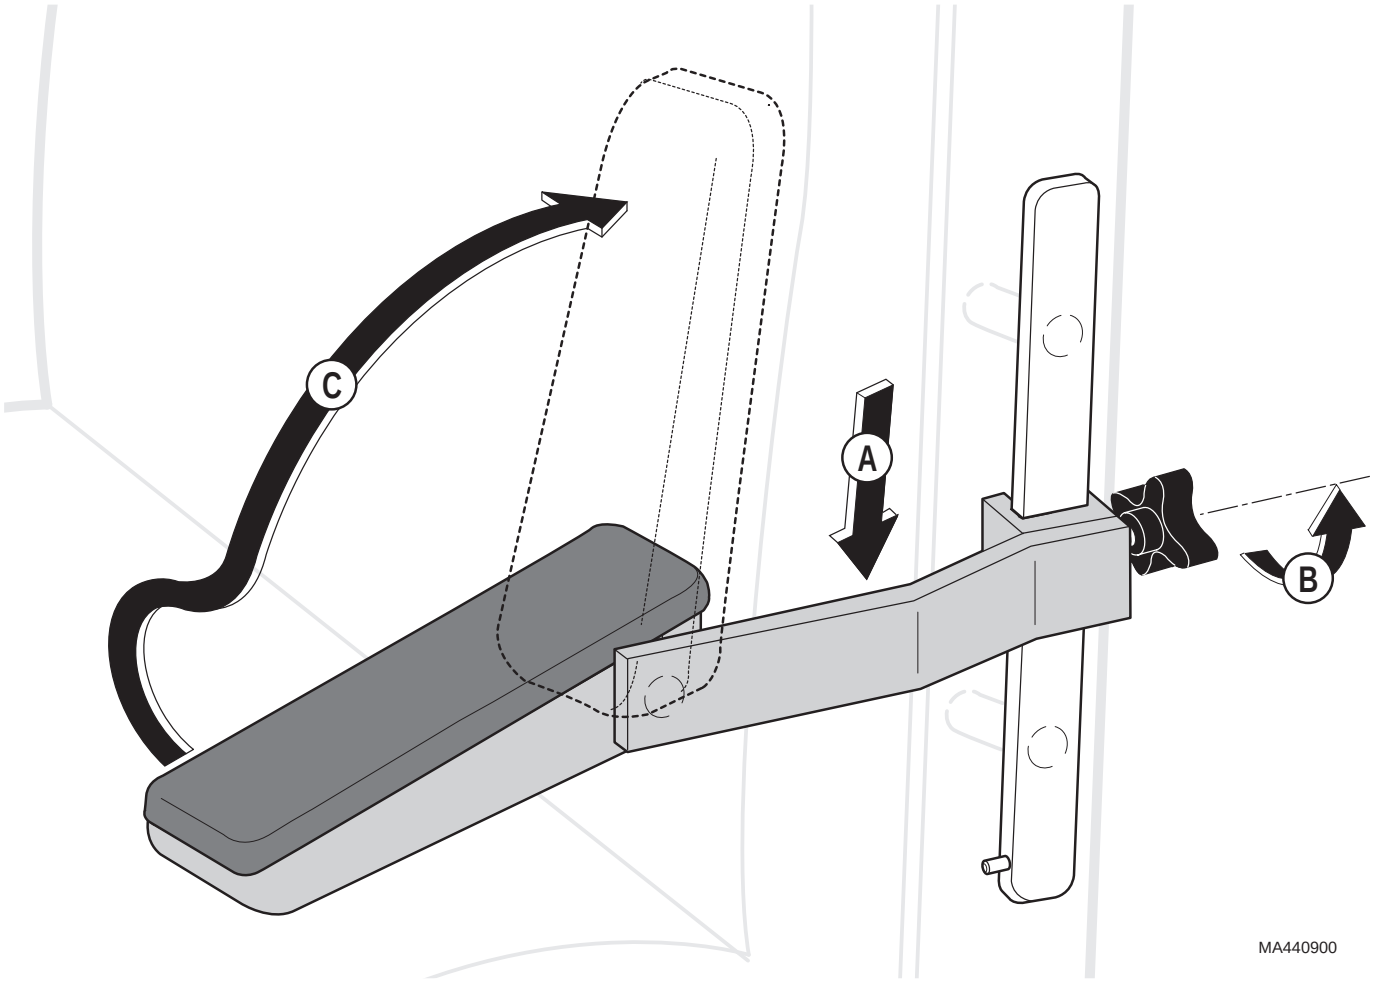

A. Slide right or left assembly onto siderail located on chair back.
B. Position at desired height, tighten knob.
C. To pivot arm assembly, move arm toward chair then; lift or lower arm.

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-0932-00 Rev. A (4/98)

© Midmark Corporation - 1998